

Posting type	Advisory
Subject	Data losses during episodes of heavy smoke
Module/Species	A/ MF, elements, f_{abs}
Sites	All
Period	All
Recommendation	Use carbon and ion data to bound MF missing during fire events.
Submitter	W.H. White, white@crocker.ucdavis.edu

Supporting information

The Teflon membrane filters used in modules A and D can clog and rupture at the high OC concentrations associated with some regional fire events. Episodes of dense smoke can thus be under-represented among days with valid mass, elemental, or light-absorption data. The degree to which such selection bias may affect a particular data analysis can usually be assessed from the ion and carbon data, as the Nylon and quartz filters used in module B and C rarely clog. ([Logistics problems](#) associated with wildfires occasionally take all four modules out of operation, but these leave more obvious gaps in the data record.)

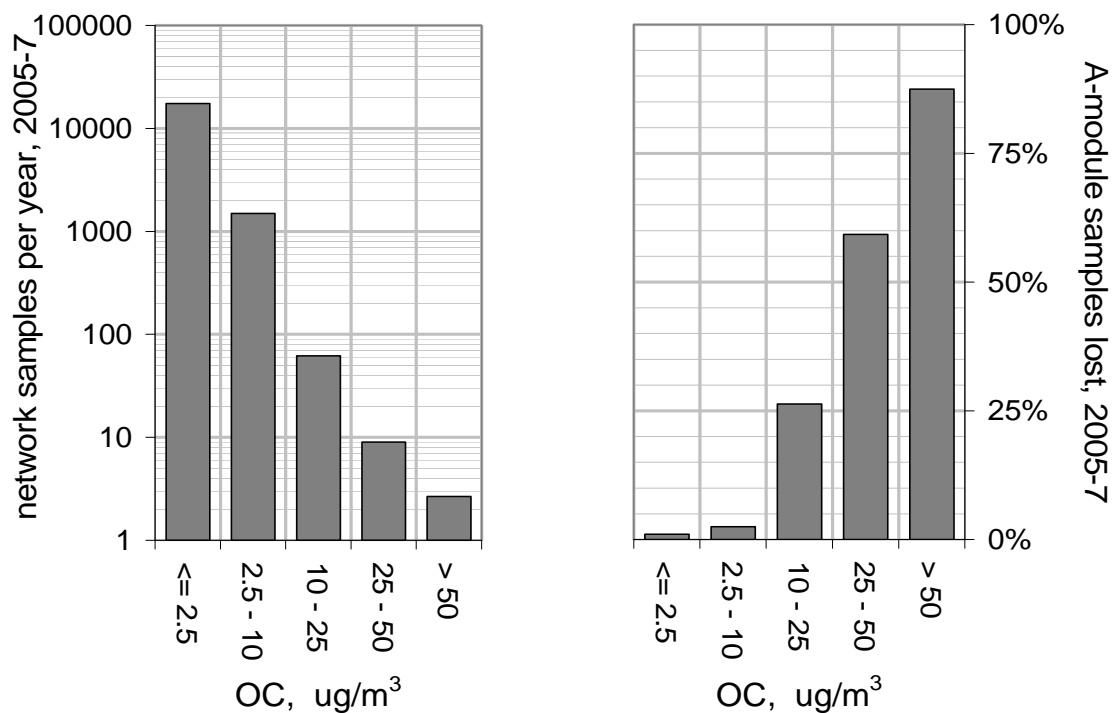


Figure 1. Mean sample recovery statistics from 2005-7 network sampling, for C module (left) and accompanying A module (right). All routine A-module samples accompanying valid C-module data are counted, including those flagged for flow and other anomalies.